



**Test Report**

NO.: BPF9JB4F41797710

Issued Date: 2021-01-27

Page 1 of 3

Applicant: E. ERHARDT Y CIA,S.A.

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Name: Meltblown Fabric

Sample Quantity/Amount: 1pcs

Sample status description: Meltblown Fabric 2 meters long from 3 different rolls

Sample Source: Send Sample

Sample Received Date: 2021-01-21

Testing Period: 2021-01-21~2021-01-27

Test Item: Please refer to next page(s)

Reference Methods: Please refer to next page(s)

Test Result: Please refer to next page(s)

Approved by:



The page below is blank



**Test Report**

NO.: BPF9JB4F41797710

Issued Date: 2021-01-27

Page 2 of 3

Test Result

Reference Methods: EN 14683: 2019 +AC: 2019

Test Item	EN 14683: 2019 +AC: 2019 Limit	Test Result			Evaluation
	Type II	A	B	C	
Differential pressure, Pa/cm <sup>2</sup>	<40	1-1	23.1	22.0	Conform
		1-2	21.9		
		1-3	21.2		
		1-4	23.0		
		1-5	20.8		
		2-1	23.2	21.4	
		2-2	23.2		
		2-3	20.8		
		2-4	19.9		
		2-5	20.1		
		3-1	20.7	21.1	
		3-2	19.5		
		3-3	21.1		
		3-4	22.7		
		3-5	21.6		
		4-1	20.7	21.6	
		4-2	21.8		
		4-3	22.3		
		4-4	21.1		
		4-5	22.0		
		5-1	19.7	20.7	
		5-2	20.7		
		5-3	21.3		
		5-4	21.5		
		5-5	20.5		
Bacterial filtration efficiency(BFE), %	≥98	No.1	99.9		Conform
		No.2	99.8		
		No.3	>99.9		
		No.4	99.9		
		No.5	99.9		




**Test Report**

NO.: BPF9JB4F41797710

Issued Date: 2021-01-27

Page 3 of 3

Sample No. &Photo:

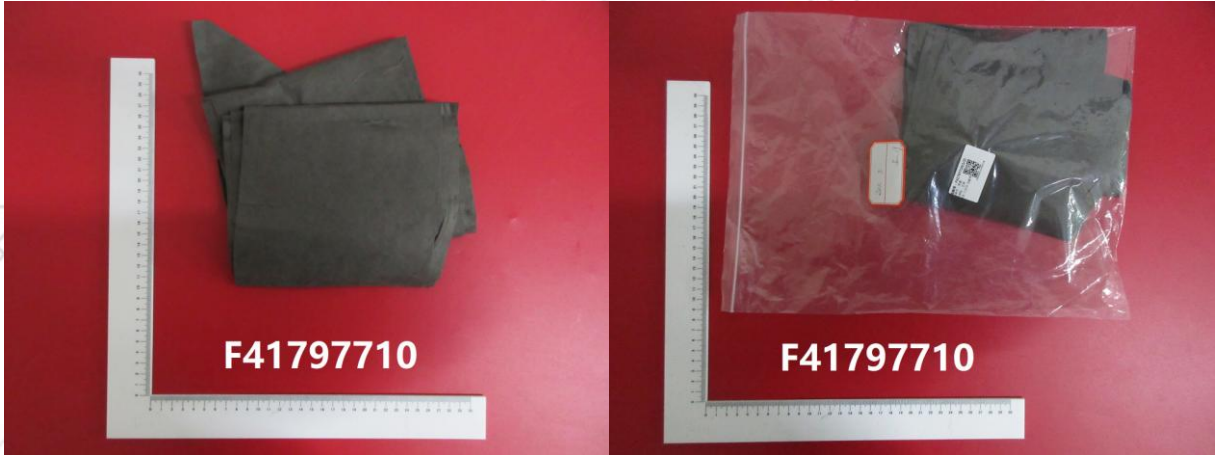

Pony authenticate the photo on original report only

——End of Report——