



**Test Report**

NO.: BPF9JB4F41796710

Issued Date: 2021-01-27

Page 1 of 3

Applicant: E. ERHARDT Y CIA,S.A.

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Name: Meltblown Fabric

Sample Quantity/Amount: 1pcs

Sample status description: Meltblown Fabric 2 meters long from 3 different rolls

Sample Source: Send Sample

Sample Received Date: 2021-01-21

Testing Period: 2021-01-21~2021-01-27

Test Item: Please refer to next page(s)

Reference Methods: Please refer to next page(s)

Test Result: Please refer to next page(s)

Approved by:



The page below is blank



**Test Report**

NO.: BPF9JB4F41796710

Issued Date: 2021-01-27

Page 2 of 3

Test Result

Reference Methods: EN 14683: 2019 +AC: 2019

Test Item	EN 14683: 2019 +AC: 2019 Limit	Test Result			Evaluation
	Type II	A	B	C	
Differential pressure, Pa/cm <sup>2</sup>	<40	1-1	22.2	22.9	Conform
		1-2	23.9		
		1-3	23.5		
		1-4	22.5		
		1-5	22.3		
		2-1	25.2	23.0	
		2-2	22.3		
		2-3	21.1		
		2-4	24.0		
		2-5	22.4		
		3-1	22.4	22.2	
		3-2	23.9		
		3-3	20.0		
		3-4	22.0		
		3-5	22.8		
		4-1	21.9	22.7	
		4-2	22.7		
		4-3	23.0		
		4-4	24.5		
		4-5	21.5		
		5-1	23.7	23.0	
		5-2	22.9		
		5-3	21.7		
		5-4	24.1		
		5-5	22.5		
Bacterial filtration efficiency(BFE), %	≥98	No.1	98.7		Conform
		No.2	>99.9		
		No.3	>99.9		
		No.4	99.9		
		No.5	99.7		




**Test Report**

NO.: BPF9JB4F41796710

Issued Date: 2021-01-27

Page 3 of 3

Sample No. &Photo:

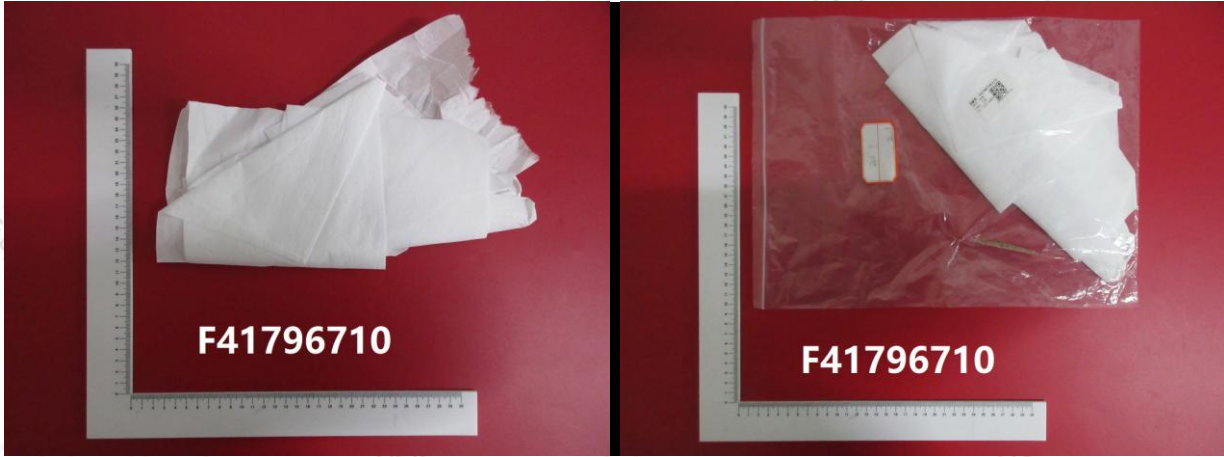

Pony authenticate the photo on original report only

——End of Report——